

Coating Thickness Gauge


Code: 86220

User Manual V2.21

Please read this manual carefully before using and reserve it for reference.

I. Product introduction

Coating thickness gauge is used for measuring the thickness of automobile paint. The automotive body shell consist of metal materials such as iron, aluminum and other non-metal materials such as carbon fiber and plastics. This coating thickness gauge can measure the thickness of car paint on iron and aluminum materials. . Moreover, it can identify not only non-metal car bodies, but also the ferrous putty layer as well as the galvanized iron.

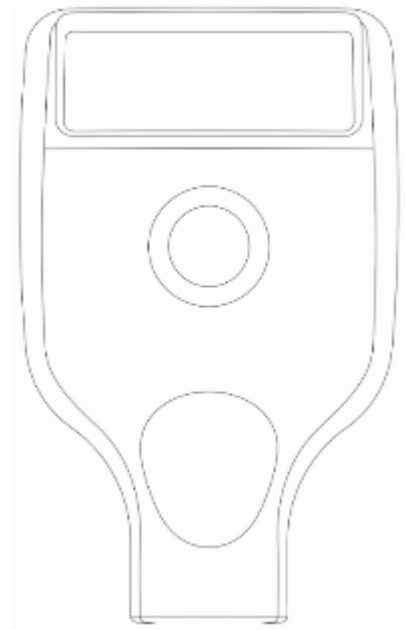

Standards for the product:

- *DIN EN ISO 2808 Paints and Varnishes-Determination of Film Thickness*
- *JJG-818-2005 Verification Regulation of Magnetic and Eddy Current Measuring Instrument for Coating Thickness*
- *GB/T 4956-2003 Non-magnetic Coatings on Magnetic Substrates-Measurement of Coating Thickness-Magnetic Method*
- *GB/T 4957-2003 Non-conductive Coatings on Non-magnetic Basis Metals-Measurement of Coating Thickness-Eddy Current*

II. Technical parameters

| | |
|------------------------|---|
| Probe tip | Ruby |
| Measuring principle | Fe: Hall Effect / NFe: Eddy current |
| Probe type | Built-in integrated probe |
| Measuring range | 0.0-5000μm |
| Resolution | 0.1μm/1μm/10μm |
| Accuracy | 0-3000μm: $\leq \pm(3\%H+2\mu m)$, H is the standard value 3000-5000μm: $\leq \pm(5\%H+2\mu m)$, H is the standard value |
| Unit | μm / mil |
| Measuring interval | 0.5s |
| Minimum measuring area | ∅ = 25mm |
| Minimum curvature | Convex:5mm / Concave:25mm |

| | |
|-----------------------------|-----------------------------------|
| Minimum substrate thickness | Fe:0.2mm / NFe:0.05mm |
| Display | 128x48 dot matrix LCD |
| Power supply | 2pcs of 1.5V AAA alkaline battery |
| Operation temperature range | -20°C-50°C |
| Storage temperature range | -20°C-60°C |
| Gauge size | 101*62*28 mm |
| Weight(with battery) | 79g |
| Supply Voltage | DC3V |
| Operating Current | 20mA |
| Operating Power Consumption | 60mW |

III. Product advantages

1. No calibration, just zero adjustment.
2. One hand operation, only one button.
3. Fast measurement, 0.5 s measuring interval.
4. Wear-proof ruby probe tip for long-term use.
5. The device can identify the ferrous putty as well as the galvanized iron substrate.
6. The gauge automatically identify the substrate and switch measurement mode rapidly.
7. Measuring non-magnetic coatings on steel or iron and measure Non-conductive coatings on non-magnetic metal substrates in one gauge.
8. Thanks to the use of the most-advanced digital probe technology, these sensors are unsusceptible to interference and provide an excellent measuring accuracy. Even variations in temperature will not affect measurement and readings remain stable to ensure a very good reproducibility over the complete measuring range.

IV. Operation

1. Power on/off

Power on:

Short press the power button to turn on the gauge. Display the version number and serial number, then

the recorded data of last measurement are displayed after the gauge is turned on.

Power off:

Long press the button to shut down the gauge, or the gauge will automatically shut down in 3 minutes without any operation.


2. Device setting

In the off state, long press the button for 3 s to enter the setting interface. After entering the setting interface, if there is no operation for more than 20 s, the instrument will automatically. Shortly press the button can select the settings; Long press the button for 3 s and less than 5 s to confirm the settings; Long press the button for 5 s, the instrument exits the setting and shuts down and the setting is invalid.

Language settings

The instrument is available in Chinese, English, Russian, Turkish, Ukrainian, German.

Setting method: In the main setting interface, short press power button to select "Language" option, long press the button for 3 seconds to confirm the selection, short press the button again to select the desired language, long press the button for 3 seconds to confirm the selection, and return to the main setting interface.

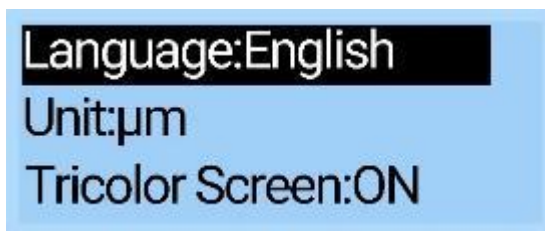


Setting interface

Unit setting

The device can be set to the metric or imperial unit, and the factory default is metric.

Setting method: In the main setting interface, shortly press the button to select "Unit". Long press the button for 3s to confirm and then enter the unit selection interface. Shortly press the button to select your unit and long press the button for 3s to confirm and back to the main setting interface.

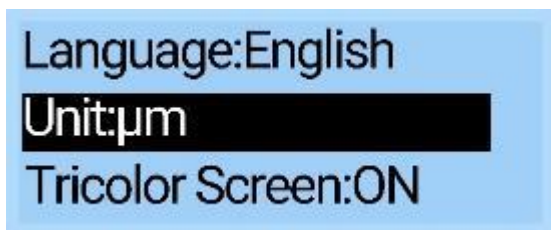

Main setting interface




Unit selection interface

Tricolor Screen Setting

The instrument can be set to ON or OFF the three-color backlight of the screen. The default setting upon factory release is ON.

Setting method: On the settings main interface, press the button shortly to select 'Tricolor Screen.' Press and hold the button for 3 seconds to enter the selection interface. Then, press the button shortly to choose to turn it on or off. Hold the button for 3 seconds to confirm the selection and exit to the settings

main interface.

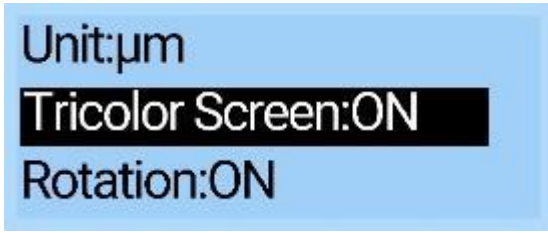

Main setting interface



Tricolor selection interface


Rotation Setting

The instrument can be set to ON or OFF the screen rotation function. The default setting upon factory release is OFF.

Rotation ON: In measurement mode, the short button is for screen rotation without history record query function.

Rotation OFF: In measurement mode, the short button is for history record query without screen rotation function.

Setting method: On the settings main interface, press the button shortly to select 'Rotation'. Press and hold the button for 3 seconds to enter the selection interface. Then, press the button shortly to choose to turn it on or off. Hold the button for 3 seconds to confirm the selection and exit to the settings main interface.

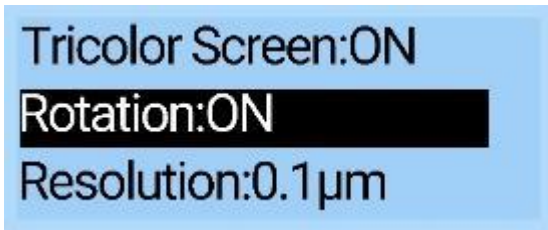

Main setting interface




Rotation selection interface

Resolution Setting


The instrument allows for resolution settings of 0.1µm, 1µm, and 10µm, and the factory default is 0.1µm.

- 0.1µm Resolution: 0.1µm: (0µm – 999.9µm), 1µm: (1000µm –5000µm).
- 1µm Resolution: 1µm: (0µm - 5000µm).
- 10µm Resolution: 10µm: (0µm - 5000µm).

Setting Method: On the main settings interface, press the button shortly to select 'Resolution.' Press and hold the button for 3 seconds to enter the selection interface. Then, press the button shortly to choose the desired resolution. Hold the button for 3 seconds to confirm the selection and exit to the settings main interface.

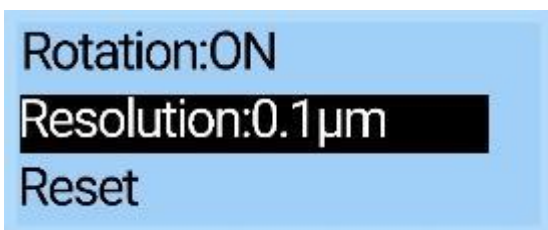


Main setting interface

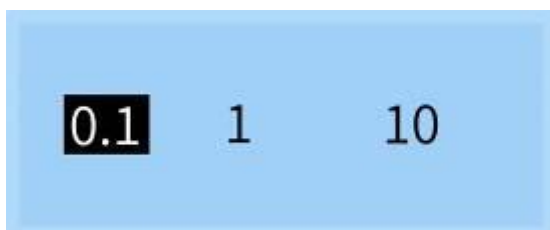

Resolution selection interface

Reset

Setting Method: On the main settings interface, press the button shortly to select 'Reset'. Press and hold the button for 3 seconds to enter the selection interface. Then, press the button shortly to choose the 'Yes' or 'No'. Hold the button for 3 seconds to confirm the selection and exit to the settings main interface.

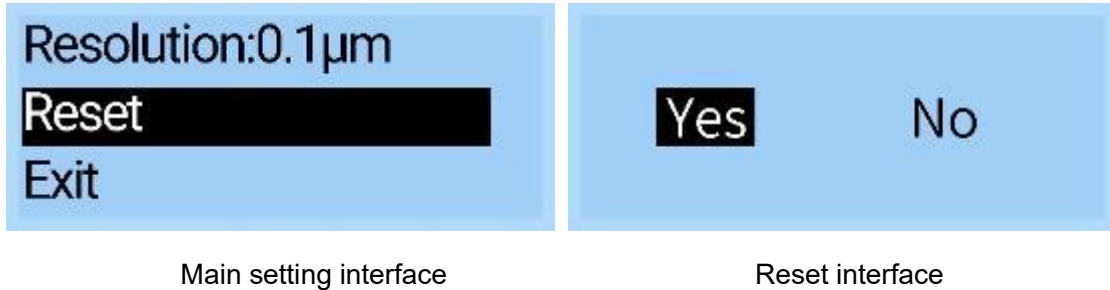

After "Reset", the default parameters are as follows:

| Item | Language | Unit | Tricolor Screen | Rotation | Resolution |
|-------|----------|------|-----------------|----------|------------|
| Reset | No Reset | µm | ON | ON | 0.1 |

Exit


In the main setting interface, short press power button to select "Exit", long press the button for 3 seconds to confirm and enter the measurement interface.

3. Zero adjustment


A zero-adjustment is required when using the gauge for the first time, after inserting new batteries, working with different materials or ambient temperature changes. Using iron-base and aluminum - base adjustment plates respectively to carry out zero adjustment. We strictly recommend carrying out the reference check on the uncoated original substrate, due to the difference of magnetic and conductive properties of the material, some measurement deviation will be caused. If this is not possible, please use the zero reference plates, there are Fe plate and NFe plate, please choose correctly according to the measuring materials.

3.1 Measuring the plate or uncoated original substrate, a measured value will be displayed on the gauge, please make sure the probe tip is placed perpendicularly and evenly on the surface.

3.2 Hold the probe still, long press the button for 3s, the gauge will display "zero reference place probe" (as shown in below picture).

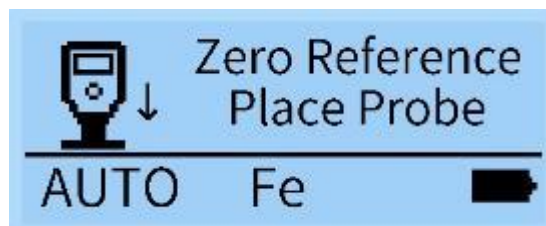

3.3 After hearing a buzzer sound, the gauge will display “Lift off probe at least 15 cm” (as shown in below picture), release the button and lift the probe away from the plate (substrate) for at least 15 cm.

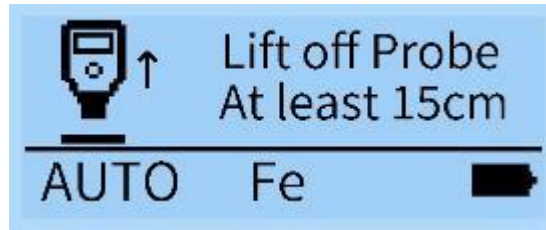

3.4 The zero adjustment completed when there is the buzzer sound again, and the LCD screen displays 0.0.



3.5 After the zero adjustment is completed, place the standard film on the plate (substrate), if the measurement value is stable and deviation from standard value within $\pm 3\mu\text{m}$, the gauge can be used normally.

Note: After the zero adjustment completed, when repeating measurement on the same spot, the reading may not always be $0\mu\text{m}$, since surface roughness, dirt, scratches etc. It might cause variances. The operation of the gauge should be correct and proficient; otherwise, it will lead to instability of the measured values.

4. Measurement

- 1) Use fingers to hold gauge where there is non-slip groove.
- 2) Press the gauge vertically on the surface of the object to be measured. Keep the gauge steady and do not tilt or shake it. The result will be shown on the screen, and there will be a buzzer.
- 3) To continue measuring, lift the gauge away from the object. Repeat the operation of step 2).
- 4) When the device identifies the ferrous putty, the buzzer alerts for two times. And the interface of the device will prompt: “Ferrous putty”. When the device identifies the galvanized iron, the substrate is displayed as “FeZn”.
- 5) Different color backlight according to the measured thickness:
 - White backlight: The measured paint thickness is $<170\mu\text{m}$;
 - Yellow backlight: The measured paint thickness is between $170\mu\text{m} - 350\mu\text{m}$;
 - Red backlight: The measured paint thickness is $>350\mu\text{m}$.

5. Check measurement records

In measurement mode, short press the button to check historical data. The gauge stores 9 sets of data. When more than 9 sets of data are stored, the earliest recorded value is automatically deleted, and No.1 is the last test data. Recorded data will not loss after powering off.

V. APP Operation

The coating thickness gauge is equipped with built-in Bluetooth communication, which can be connected to the gauge through the mobile app.

1. Mobile APP installation and use

- 1) Mobile APP installation: Scan the QR code on the instrument with your cell phone's browser or the system's own scanning function, and follow the instructions to download and install coating thickness gauge software; iPhones can be installed by searching for "Coating Thickness Gauge" in the App Store. After installation, the icon of "Coating Thickness Gauge" will appear on the desktop of your cell phone as shown in the picture below.



- 2) Connect the device: Open the APP. If there is no bound Bluetooth device, then enter the Bluetooth setting interface. Click "Start Searching", prompt "Searching for device..." and list the available Bluetooth devices that are searched; click the "Stop Searching" button to stop searching for Bluetooth devices. Selecting gauge serial number will bind the selected gauge (prompt: each gauge has a unique serial number). After the connection is successful, it will automatically enter into the main measurement interface and Bluetooth icon will be displayed at the bottom right of the gauge screen. If the APP has a bound Bluetooth device, automatically search and connect the bound Bluetooth device. When the connection is successful, it will automatically enter the "Measure" interface.

VI. Attentions

1. The device must be zero adjusted respectively with the iron-base and aluminum-base zero adjustment plates. Otherwise, there may be abnormal identifications of the ferrous putty and galvanized iron substrate.
2. Some car bodies may be misjudged as iron-zinc car bodies due to the base material.
3. Do not slide the probe on the car surface, which will result in damage to the paint and the gauge.
4. Please keep the car paint surface clean, the dust and dirt on the paint surface will affect the measurement accuracy.

5. When the gauge displays low battery, the battery needs to be replaced.

VII. Packing list

| No. | Description | Quantity | Unit |
|-----|-----------------------------|----------|------|
| 1 | Coating Thickness Gauge | 1 | Set |
| 2 | Fe zero-adjustment plate | 1 | pcs |
| 3 | NFe zero-adjustment plate | 1 | pcs |
| 4 | Standard film | 1 | pcs |
| 5 | User manual | 1 | pcs |
| 6 | Certificate / Warranty card | 1 | pcs |

VIII. Service

1. The gauge has one-year warranty. If the gauge works abnormally, please send the whole gauge to our company for maintenance.
2. Provide users with spare parts and lifelong maintenance services.
3. Provide the users with the gauge calibration service.
4. Free technical support for long term.